BD Vacutainer® Push Button Blood Collection Set with Pre-Attached Holder

PRZEZNACZENIE/WSKAZANIA DO STOSOWANIA
Zestaw do pobierania krwi BD Vacutainer® Push Button Blood Collection Set with Pre-Attached Holder firmy Becton Dickinson and Company (BD) jest przeznaczony do jednorazowego użytku do pobierania krwi z powyższą krótkotrwałą ochroną na pojedyncze pobranie krwi przy użyciu probówek próżniowych BD Vacutainer®. Zestaw jest przeznaczony do użytku przez profesjonalistów służby zdrowia, w tym od pacjentów z tym od pacjentów z trudnymi dostępami, u których mogą występować małe, kruche żyły oraz pacjentów z podejrzeniem mukowiscydozy (choroba genetyczna). Klub badania na poziomie krwi. W przypadku użycia bez mechanizmu adaptacyjnego Luer wymaga zamocowania igły do uchwytu przed użyciem. Zestaw nie jest przeznaczony do użytku w laboratorium. Ten wyrób może być używany przez pracowników służby zdrowia z działalnościowemi w zakresie wiedzenia do krótkotrwałych, pojedynczych wlewów z urządzeniami wewnątrznaczyniowymi i/lub w celu pobierania próbek krwi, zgodnie z zaleceniami lekarza. Nie należy pozostawiać wyrobu w miejscu wlotu i powinien on być chroniony przed bezpośrednim kontaktem z pacjentem.

Zestaw do zbierania krwi BD Vacutainer® Push Button Blood Collection Set with Pre-Attached Holder firmy Becton Dickinson and Company (BD) jest przeznaczony do jednorazowego użytku do pobierania krwi z powyższą krótkotrwałą ochroną na pojedyncze pobranie krwi przy użyciu probówek próżniowych BD Vacutainer®. Zestaw jest przeznaczony do użytku przez profesjonalistów służby zdrowia, w tym od pacjentów z trudnymi dostępami, u których mogą występować małe, kruche żyły oraz pacjentów z podejrzeniem mukowiscydozy (choroba genetyczna). Klub badania na poziomie krwi. W przypadku użycia bez mechanizmu adaptacyjnego Luer wymaga zamocowania igły do uchwytu przed użyciem. Zestaw nie jest przeznaczony do użytku w laboratorium. Ten wyrób może być używany przez pracowników służby zdrowia z działalnościowemi w zakresie wiedzenia do krótkotrwałych, pojedynczych wlewów z urządzeniami wewnątrznaczyniowymi i/lub w celu pobierania próbek krwi, zgodnie z zaleceniami lekarza. Nie należy pozostawiać wyrobu w miejscu wlotu i powinien on być chroniony przed bezpośrednim kontaktem z pacjentem.

OPIS
- BD Vacutainer® Blood Transfer Device w przypadku połączenia krwi do strzykawki.
- Urządzenia w zbiorem Luer do podłączenia dozujących (25 cm) połączenia krwi do strzykawki.

Wyrób ogólny zgodnie z procedurami pisemnej w zakresie wiedzenia dożylnego i krótkotrwałego podania dożylnego. Dzięki wyrobowi podano dożylnego.

Procedura dla połączenia krwi (patrz schemat 1)
1. Sprawdzić, czy zestaw należy do użytku przed datą ważności przynależności do medycznego zabiegu Luer.
2. Zdejmij opakowanie, zdecydowanie mocno wkłuć dożylnego wkłuć.
3. Wybierz właściwe dożylne, trzymając dowolne skrzydła motylka lub bezpośrednio.
4. Podłącz probówkę.
5. Wprowadzić probówkę, trzymając dowolne skrzydła motylka lub bezpośrednio.
6. Odłączyć strzykawkę i wyrzucić igłę oraz wyjąć do dopuszczonego do użytku pojemnika na odpady stosowanego zgodnie z lokalnymi wymaganiami.

Sposób użytkowania (patrz schemat 2)
1. Zdejmij osłonę igieł i przykręć strzykawkę.
2. Otwórz zacisk.
3. Sprawdź udrożnić i dużo krwi na miejscu wkłuciowym.
4. Zamknij zacisk.
5. Wyjmij strzykawkę z zestawu.
6. Wyjmij probówkę z uchwytu.
7. Wyjmij probówkę z uchwytu.
8. Wyjmij probówkę z uchwytu.
9. Wyjmij probówkę z uchwytu.
10. Wyjmij probówkę z uchwytu.

Ostrzeżenia
- W przypadku wkłucia z użyciem mechanizmu adaptacyjnego Luer należy zamocować igłę do uchwytu przed użyciem.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.
- Nie należy stosować igły podczas wkłucia.

Środki ostrożności
- Produkt należy używać w temperaturze pokojowej.
- Stosować standardowe środki ostrożności.
- Klauzule elementy obejmujące igłami/igłami, czyszczenie skrzepów, stosowanie zacisku ochronnego. Produkt należy zutylizować zgodnie z lokalnymi wymaganiami.
- Nie należy stosować wyrobu, jeśli opakowanie wskazuje oznaki naruszenia sterylności.
- Należy stosować technikę aseptyczną, aby zminimalizować ryzyko zakażenia.
- Wyrobów użyć zbiorczej zbiorczej igły na miejscu wkłucia dożylnego

BD Vacutainer®
Push Button
Blood Collection Set with Pre-Attached Holder

CE 0050 MD UA.TR.116 Rx Only STERILE R Cobalt eifu.bd.com

REF 367354
REF 367355
REF 367352*
REF 368656*
REF 368657
REF 368658
REF 368659*

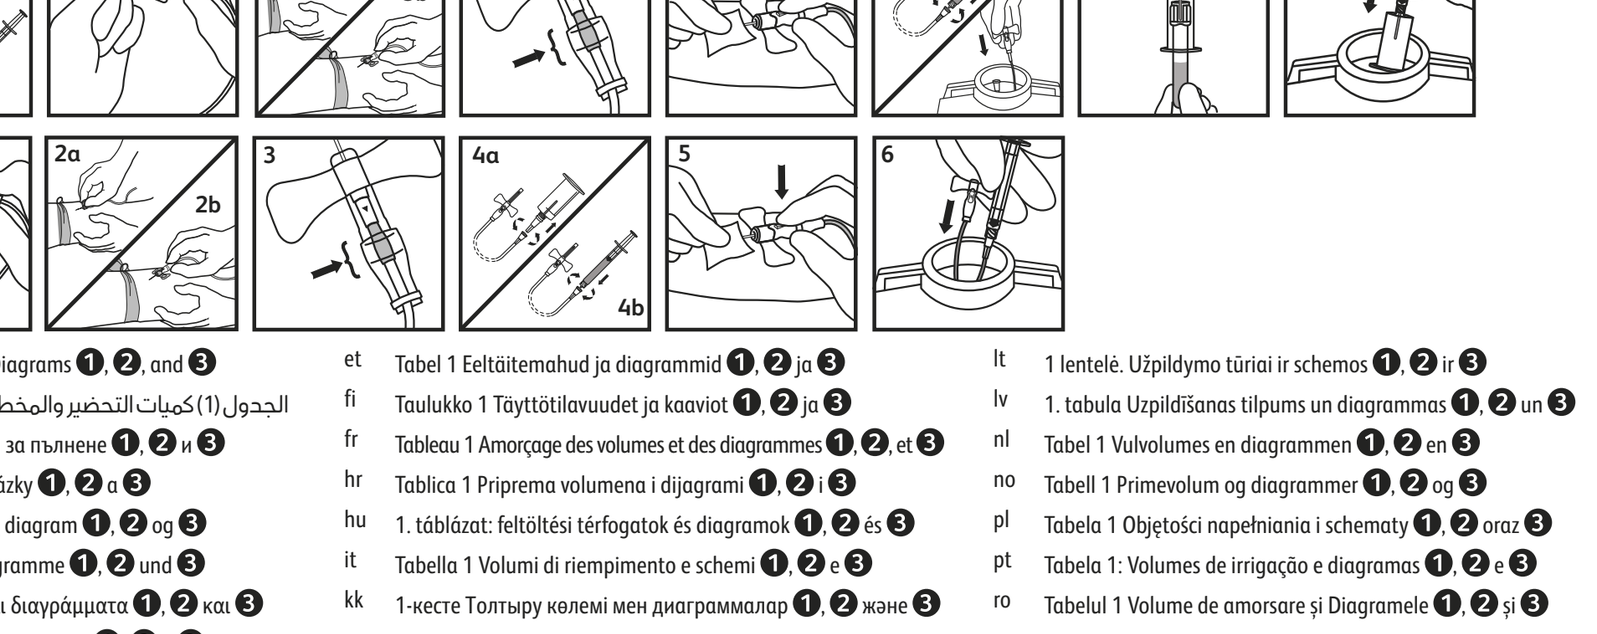

Table 1: Priming Volume		
Gauge (G)	Tubing Length (inch/mm)	Volume (mL)
21	7/177.8	0.228
23	7/177.8	0.225
25	7/177.8	0.224
21	12/304.8	0.353
23	12/304.8	0.350
25	12/304.8	0.349

en Table 1 Priming Volumes and Diagrams ❶, ❷, and ❸
ar الجدول (1) كميات التحضير والمخططات التوضيحية ❶، ❷، و❸
bg Таблица 1 Обеми и диаграми за пълнене ❶, ❷ и ❸
cs Tabulka 1 Objemy plnění a obrázky ❶, ❷ a ❸
da Tabel 1 Fyldningsvolumener og diagram ❶, ❷ og ❸
de Tabelle 1 Füllvolumen und Diagramme ❶, ❷ und ❸
el Πίνακας 1 Όγκοι πλήρωσης και διαγράμματα ❶, ❷ και ❸
es Tabla 1 Volúmenes de purga y diagramas ❶, ❷ y ❸
et Tabel 1 Eeltäitemahud ja diagrammid ❶, ❷ ja ❸
fi Taulukko 1 Täyttötilavuudet ja kaaviot ❶, ❷ ja ❸
fr Tableau 1 Amorçage des volumes et des diagrammes ❶, ❷, et ❸
hr Tablica 1 Priprema volumena i dijagrami ❶, ❷ i ❸
hu 1. táblázat: feltöltési térfogatok és diagramok ❶, ❷ és ❸
it Tabella 1 Volumi di riempimento e schemi ❶, ❷ e ❸
kk 1-кесте Толтыру көлемі мен диаграммалар ❶, ❷ және ❸
lt 1 lentelė. Užpildymo tūriai ir schemos ❶, ❷ ir ❸
lv 1. tabula Uzpildīšanas tilpums un diagrammas ❶, ❷ un ❸
nl Tabel 1 Vulvolumes en diagrammen ❶, ❷ en ❸
no Tabell 1 Primevolum og diagrammer ❶, ❷ og ❸
pl Tabela 1 Objętości napełniania i schematy ❶, ❷ oraz ❸
pt Tabela 1: Volumes de irrigação e diagramas ❶, ❷ e ❸
ro Tabelul 1 Volume de amorsare și Diagramele ❶, ❷ și ❸
ru Таблица 1. Объемы заполнения и схемы ❶, ❷ и ❸
sk Tabuľka 1 Objemy naplnenia a obrázky ❶, ❷ a ❸
sl Tabela 1: Količine za zapolnitev ter diagrami ❶, ❷ in ❸
sr Tabela 1 Količine za punjenje i dijagrami ❶, ❷, i ❸
sv Tabell 1 Fyllningsvolymer och Diagram ❶, ❷ och ❸
tr Tablo 1 Hazırlama Hacimleri ve Şema ❶, ❷ ve ❸
uk Таблиця 1. Об'єми первинного заповнення та рисунки ❶, ❷ і ❸
zh 表 1 注液量和图 ❶、❷ 和 ❸

en

INTENDED USE/INDICATIONS FOR USE

The BD Vacutainer® Push Button Blood Collection Set with Pre-Attached Holder is a sterile, multi-sample, single-use fixed winged blood collection set intended for use in the general population by healthcare professionals experienced with venipuncture to obtain blood specimens from patients, including those with difficult vein access who may have small, fragile, and/or non-palpable veins, into evacuated blood collection tubes and/or blood culture bottles. When used without the male Luer adapter, the device allows the clinician to obtain a blood specimen from the female Luer connector with a syringe, if necessary. The device can be used by healthcare professionals with infusion experience for short-term, single infusions with consideration given to patient size and appropriateness for the solution being infused. The device is not to be left in place and is to remain under the direct supervision of a clinician.

The recommended use of the device is to activate the needle safety feature prior to removal from the venipuncture site. The retraction of the intravenous (IV) end of the needle aids in the prevention of accidental needlestick injury.

NEEDLE GAUGE SELECTION

The healthcare professional should select the needle gauge depending on:

- the patient condition (such as age, weight, pre-existing conditions),
- physical characteristics of the vein (such as size, location, and accessibility),
- for blood collection, the volume of blood needed to be collected,[1,2]
- for infusion, the prescribed therapy and patient need.[3]

Choose the needle gauge that fits comfortably into the most prominent vein with little discomfort. The following are recommended needle gauges for venipuncture or infusion procedures for different age groups;

- 21G is recommended for adults[1]
- 23G and 25G** are recommended for adults, pediatrics, elderly or patients with small, fragile veins, and neonates.[1,2]

**25G may be associated with an increased risk of hemolysis[1]

PERFORMANCE CHARACTERISTICS AND CLINICAL BENEFITS

1. Single handed, in-vein needle retraction aids in the prevention of an accidental needlestick and blood splatter.
2. Flashback visualization indicates vein entry.
3. Non-patient needle sleeve enables a multi-sample blood collection.

Required Equipment Provided

- BD Vacutainer® Push Button Blood Collection Set with Pre-Attached Holder.

Required Equipment Not Provided

- BD BACTEC™ brand blood culture bottles and/or BD Vacutainer® brand blood collection tubes, as dictated by test request.
- Approved biohazard container and other supplies, such as tourniquet, gloves, skin disinfectant, and sterile gauze.
- BD Vacutainer® Blood Transfer Device for syringe blood collection.
- Devices with Luer connection for IV administration and syringe blood collection.

Follow your facility's procedures for venipuncture for blood collection and short term IV administration. General guidance is provided below.

Procedure For Blood Collection (see Diagram ❶)

1. Check to ensure that the female Luer adapter Ⓐ is securely attached to the male Luer adapter Ⓑ.
2. Apply tourniquet, disinfect the venipuncture site and remove needle sheath.
3. Perform venipuncture by holding either wings or body of the device.
4. Observe for the presence of blood in the flash chamber prior to collecting blood specimen to indicate venous access. Release tourniquet as soon as blood flow is established. Collect blood specimen(s) in accordance with the tube manufacturer's order of draw and recommended fill volumes and/or the blood culture bottle manufacturer's instructions for use.
5. Retract the needle: Place sterile gauze over the venipuncture site while the needle is still in the vein and then depress the button. The needle will slide out of the venipuncture site and lock into place. Do not impede needle retraction. Cover the puncture site with a sterile gauze and apply pressure.
6. Dispose of all used materials in an approved biohazard container.

Procedure For Blood Collection Using A Syringe (see Diagram ❷)

1. Remove the Luer Adapter and attach syringe.

Follow Blood Collection Steps 2–5.

6. Detach syringe and dispose of needle and tubing in an approved biohazard container.
7. Use the BD Vacutainer® Blood Transfer Device to transfer blood from the syringe to the evacuated tube(s) in accordance with the tube manufacturer's order of draw and recommended fill volumes and/or the blood culture bottle manufacturer's instructions for use.
8. Dispose of syringe and all used materials in an approved biohazard container.

Procedure For Short Term IV Administration (see Diagram ❸)

(Up to 2 hours under direct supervision of clinician)

- When securing the device, tape the wings. Note: Taping over the button and applying pressure may cause the needle to retract.
- Prime set if necessary, in accordance with your facility's procedure (See Table 1, Priming Volume. Column 1 is gauge, column 2 is tubing length in inches/millimeters (mm) and column 3 is in mL).

1. Apply tourniquet, disinfect the venipuncture site and remove needle sheath.
2. Perform venipuncture by holding either wings or body of the device.
3. Observe for the presence of blood in the flash chamber and release tourniquet.
4. (a) Remove the Luer Adapter.
   (b) Attach IV line or syringe to the female Luer connector, ensure that there is no air in the system and start infusion.
   • The device should be changed in accordance with your facility's procedure and should not be used for longer than 2 hours.
5. Retract the needle. Place sterile gauze over the venipuncture site while the needle is still in the vein and then depress the button. The needle will slide out of the venipuncture site and lock into place. Do not impede needle retraction. Cover the puncture site with a sterile gauze and apply pressure.
6. Dispose of all used materials in an approved biohazard container.

SAFETY PRECAUTIONS AND WARNINGS

Precautions

1. Use product at room temperature.
2. Practice Standard Precautions.
   • Key elements include hand hygiene, cleaning of the environment, use of gloves, eye protection, other personal protective equipment, waste management and engineering controls to protect from blood splatter, blood leakage, and potential exposure to infectious agents.
   • Practice aseptic technique to minimize the risk of healthcare-associated infections.
3. Prolonged tourniquet time greater than 1–2 minutes may cause hemoconcentration which can impact test results.
4. For all infusates, adhere to all contraindications, warnings, precautions, and instructions for use, as specified by their manufacturer(s).
5. For infusion, balance the risk of infiltration against the venous trauma when choosing a needle gauge.
6. Use only compatible male Luer connectors. Non-compatible Luer connectors may cause leakage, hemolysis and incorrect draw volumes.
7. Do not over-tighten Luer connections as damage may occur.
8. Using a syringe to draw blood may result in increased hemolysis.
9. Do not obstruct needle during activation. Visually confirm that the needle point is completely covered.
10. Male Luer adapter and holder are not intended to be separated.
11. The device is designed and intended for use in combination with BD Vacutainer® brand blood collection tubes, BD BACTEC™ brand blood culture bottles, and BD Vacutainer® Blood Transfer Device. The safety and performance of the device has not been established for use in combination with other devices.
12. Incomplete fill of tubes/blood culture bottles could lead to erroneous results which may potentially result in improper diagnosis or treatment.
13. This device contains the following substance defined as CMR 1B, in a concentration above 0.1% weight by weight: Cobalt, CAS Number 7440-48-4 and EC Number 231-158-0. Current scientific evidence supports that medical devices manufactured from cobalt alloys or stainless steel alloys containing cobalt do not cause an increased risk of cancer or adverse reproductive effect. Note: For more information, please consult the European Chemicals Agency website: echa.europa.eu/home.

Warnings

1. Obtain appropriate medical attention in the event of any exposure to biologic samples (for example, through a puncture injury), since samples may transmit viral hepatitis, HIV (AIDS), or other infectious diseases. Utilize any safety engineered feature if the blood collection device provides one.
2. Discard all blood collection "sharps" in puncture resistant biohazard containers approved for their disposal.
3. Do not use if foreign matter is present as it may lead to infection, allergic or toxic reaction. Unintended device material or infusate exposure into the body can lead to infection, allergic or toxic reaction.
4. Intended for single-use only. Reuse may lead to infection or other illness/injury.
5. Activation of the device while the needle is still in the venipuncture site is recommended. Activation of the device after the needle is removed from the site should be performed away from self and others to avoid exposure to blood or IV fluid splatter.
6. Do not use device after its expiration date.
7. Potential adverse events associated with phlebotomy, infusion, or device malfunction such as, but not limited to, moderate discomfort, bruising, hematoma, pain, infection, hemoconcentration, nerve/vein/tissue damage, edema, accidental arterial puncture, iatrogenic anemia, vasovagal reaction, syncope, diaphoresis with near syncope, petechiae, allergies, thrombosis, phlebitis, thrombophlebitis, loss of consciousness with tonic-clonic seizures, extravasation, infiltration, or air embolism may occur due to patient physiological characteristics, chosen venipuncture/anatomic site, and clinical experience of the healthcare professional.

EU Only: Users should report any serious incident related to the device to the Manufacturer and National Competent Authority.

Outside EU: Contact your local BD representative for any incident or inquiry related to this device.

TECHNICAL SERVICES AND SUPPORT

In the United States, contact BD at 1-800-638-8663 OPT 3 or bd.com. For regions outside of the United States, contact your local BD representative or bd.com.

This instructions for use is also available electronically on eifu.bd.com.

For U.S. patents that may apply, see bd.com/patents.

REFERENCES

1. World Health Organization (2010). WHO Guidelines on Drawing Blood: Best Practices in Phlebotomy. World Health Organization.
2. Clinical Laboratory and Standards Institute (2017). GP41 Collection of Diagnostic Venous Blood Specimens, 7th Edition. Clinical and Laboratory Standards Institute.
3. Infusion Nurses Society. Infusion Therapy Standards of Practice, 8th Edition 2021.